



US00D782658S

(12) **United States Design Patent**
Young

(10) **Patent No.:** **US D782,658 S**

(45) **Date of Patent:** **** Mar. 28, 2017**

(54) **AIRWAY DEVICE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **INDIAN OCEAN MEDICAL INC.,**
Mahe (SC)

DE 19734821 A1 2/1999
GB 1399093 6/1975

(Continued)

(72) Inventor: **Peter J. Young,** Roydon King's Lynn
(GB)

OTHER PUBLICATIONS

(73) Assignee: **Indian Ocean Medical Inc.,** Mahe
(SC)

Evans, L. et al., "Comparison of the LoTrach and the Portex Soft Seal Cuff: Tracheal Wall Pressure and Fluid Leakage in a Benchtop Study and a Clinical Study", 27th International Symposium on Intensive Care and Emergency Medicine, Mar. 27-30, 2007, published Mar. 22, 2007 in Critical Care, 11 (Suppl 2): p215doi:10.1186/cc5375, Brussels, Belgium, BioMed Central Ltd.

(Continued)

(**) Term: **15 Years**

(21) Appl. No.: **29/534,593**

(22) Filed: **Jul. 30, 2015**

(30) **Foreign Application Priority Data**

Primary Examiner — David Muller

Feb. 2, 2015 (EP) 001429815

(74) *Attorney, Agent, or Firm* — Ostrager Chong Flaherty & Broitman P.C.

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/112**

(58) **Field of Classification Search**
USPC D24/112-114, 108, 133, 130, 127, 186;
606/181, 185; 604/264, 272, 187, 181,
604/184, 227; 600/101, 139, 143;
128/200.24, 207.14, 207.15
CPC A61M 25/00; A61M 39/00; A61M 27/00;
A61M 25/0043; A61M 25/0067; A61M
25/0097

See application file for complete search history.

(57) **CLAIM**

I claim the ornamental design for an airway device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front and left side perspective view of the new design;
FIG. 2 is a bottom, rear and right side perspective view thereof in a different configuration;
FIG. 3 is a front side view thereof in a different configuration;
FIG. 4 is a right side elevation view thereof;
FIG. 5 is a left side elevation view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken lines in the Figures form no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

3,407,817 A 10/1968 Galleher, Jr.
3,734,100 A 5/1973 Walker et al.
3,880,168 A 4/1975 Berman
3,884,242 A 5/1975 Bazell et al.
4,056,104 A 11/1977 Jaffe
4,305,392 A 12/1981 Chester

(Continued)

1 Claim, 6 Drawing Sheets

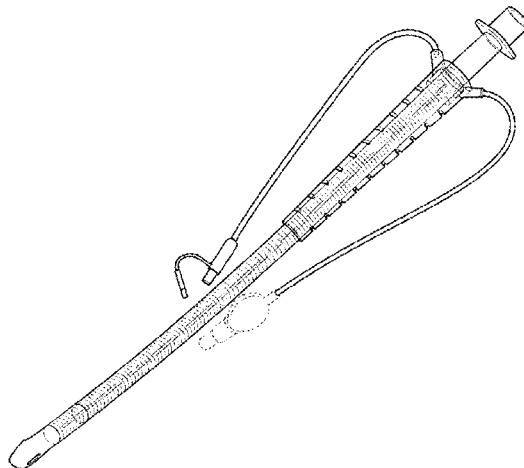

(56)

References Cited

U.S. PATENT DOCUMENTS

4,327,721 A 5/1982 Goldin et al.
 4,393,872 A * 7/1983 Reznik A61B 10/06
 600/565
 D328,128 S * 7/1992 Fox D24/112
 5,143,062 A 9/1992 Peckham
 5,146,916 A 9/1992 Catalani
 D338,063 S * 8/1993 Idowu D24/111
 5,311,864 A 5/1994 Huerta
 5,334,148 A 8/1994 Martin
 5,501,215 A 3/1996 Huerta
 5,605,147 A * 2/1997 Truthan A61M 16/0463
 128/203.12
 5,803,080 A 9/1998 Freitag
 5,957,134 A 9/1999 Lee
 5,976,153 A 11/1999 Fischell et al.
 6,062,223 A 5/2000 Palazzo et al.
 6,093,142 A 7/2000 Ciamacco, Jr.
 6,135,111 A * 10/2000 Mongeon A61M 16/04
 128/200.21
 6,568,388 B2 * 5/2003 Christopher A61M 16/0488
 128/200.26
 6,723,113 B1 4/2004 Shkolnik
 7,360,540 B2 4/2008 Brain et al.
 8,220,462 B2 * 7/2012 Coates A61M 16/0465
 128/207.14
 8,408,210 B2 * 4/2013 Curley A61M 16/04
 128/207.15
 8,535,297 B2 * 9/2013 Kogiso A61B 17/122
 600/139
 8,961,402 B2 * 2/2015 Okamoto A61B 1/0052
 600/139
 8,967,204 B2 * 3/2015 Konstorum A61M 25/0138
 138/119

9,023,314 B2 * 5/2015 O'Neil A61M 16/04
 128/207.14

2002/0043266 A1 4/2002 Toti et al.
 2003/0070682 A1 4/2003 Wilson et al.
 2004/0079376 A1 4/2004 Melker

FOREIGN PATENT DOCUMENTS

GB 1414344 11/1975
 GB 1526286 9/1978
 GB 2008140 5/1979
 GB 2324735 4/1998
 WO 9938548 A1 5/1999
 WO 03061747 A1 7/2003
 WO 2005118039 A1 12/2005
 WO 2015063459 A1 5/2015

OTHER PUBLICATIONS

Evans, L. et al., "Preventing Iatrogenic Air Embolism in the Intensive Care Unit", published on EMDT—European Medical Device Technology (<http://www.emdt.co.uk>) on May 1, 2007.
 Santhirapala, R. et al., "Tracheal Wall Pressures in the Clinical Setting: Comparing Portex Soft Seal and Lotrach Cuffs", 28th International Symposium on Intensive Care and Emergency Medicine, Mar. 18-21, 2008, published Mar. 13, 2008 in Critical Care, 12 (Suppl 2): p339doi:10.1186/cc6560, Brussels, Belgium, BioMed Central Ltd.
 Young, Peter J. et al., "A Low-Volume, Low-Pressure Tracheal Tube Cuff Reduces Pulmonary Aspiration", Crit Care Med 2006, vol. 34, No. 3, Mount Prospect, Illinois.
 Young, P. "The LoTrach™, A Tracheal Tube for Critical Care," The Journal of the Intensive Care Society, Spring 2007, London, U.K.

* cited by examiner

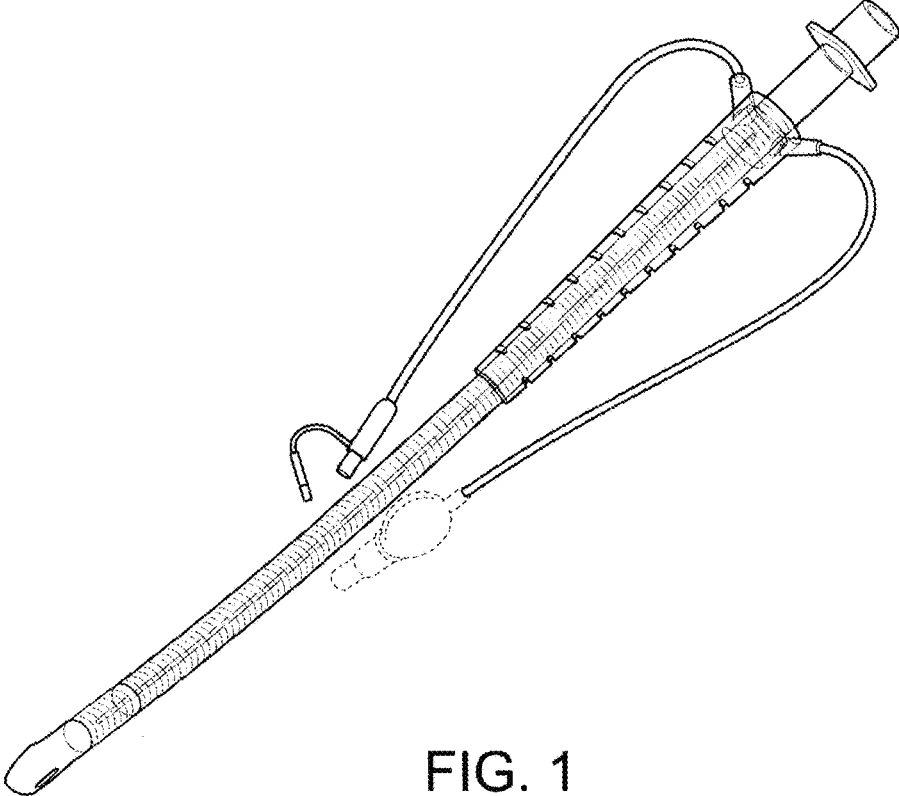


FIG. 1

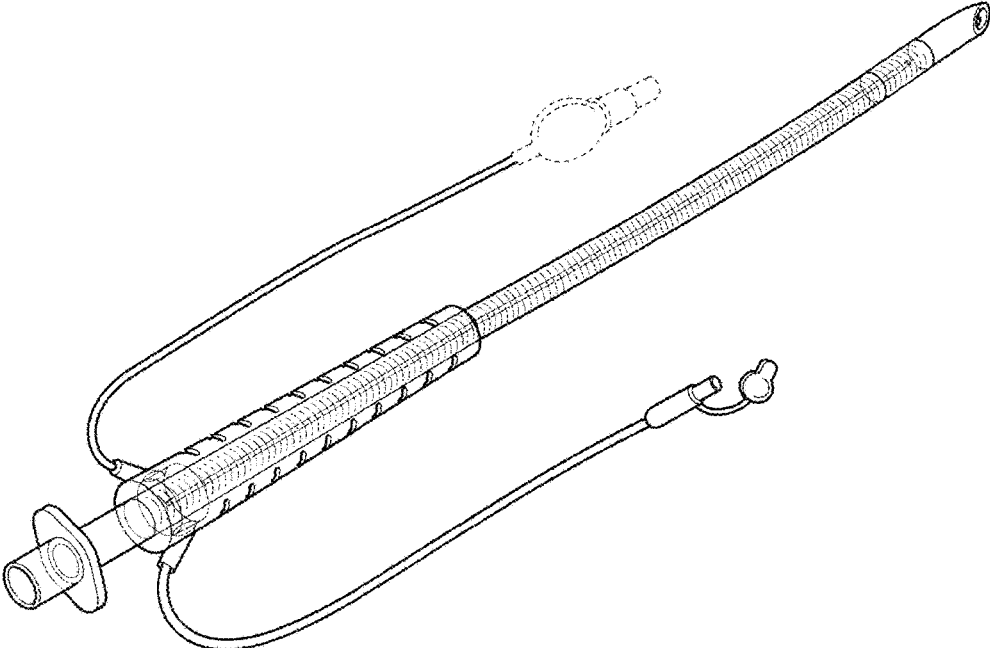


FIG. 2

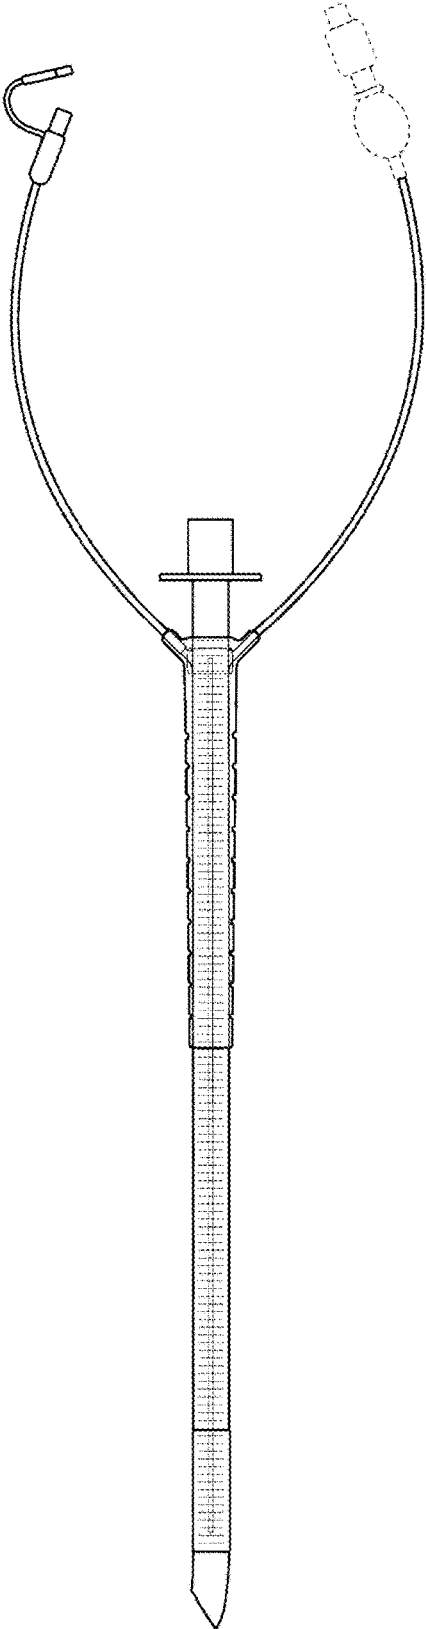


FIG. 3




FIG. 4



FIG. 5

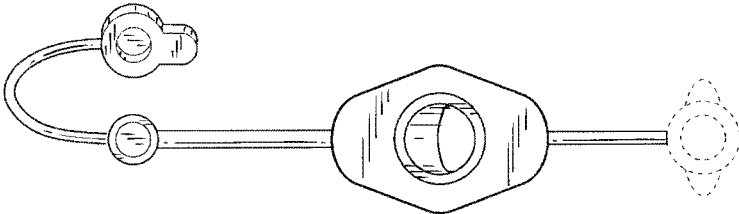


FIG. 6

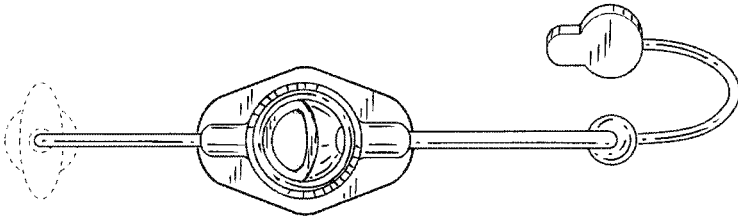


FIG. 7